OCUFY BEEP

Setup instructions.

STEP 1

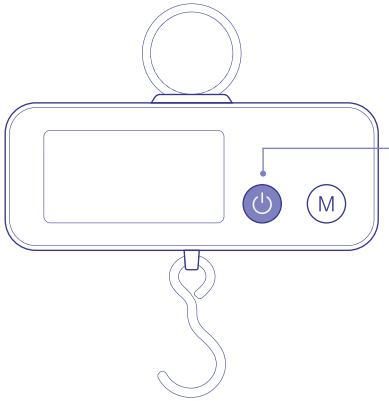

Turn on the device
without anything hanging.
– Dont hang the B.S.S. yet!

STEP 2

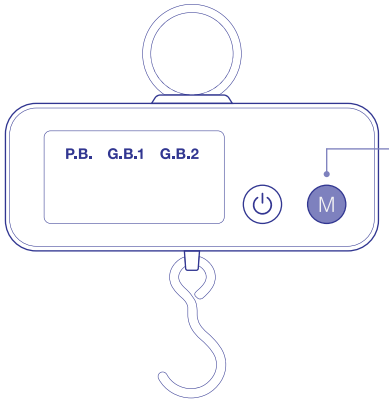

Choose the desired mode:

P.B. *– Plastic bottle. For all plastic B.S.S. or Ringer lactate bags/bottles.*

G.B.1 *– Glass Bottle 1. For Bausch + Lomb B.S.S. glass bottle or similar.*

G.B.2 *– Glass Bottle 2. For Alcon B.S.S. glass bottle or similar.*

STEP 3

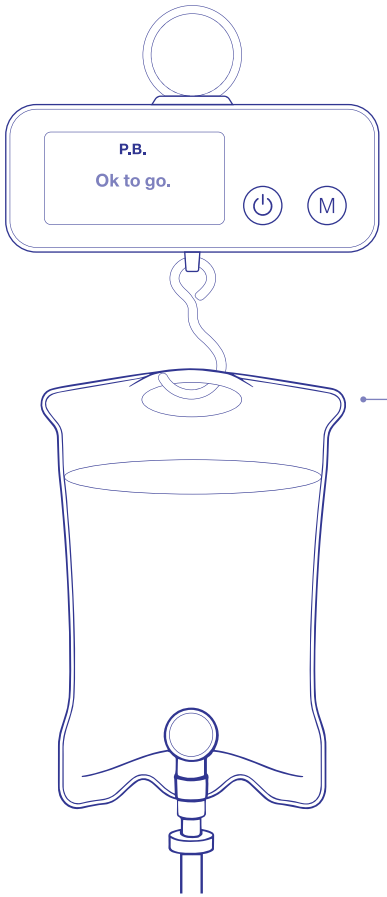

Hang the device from the infusion pole, the B.S.S. or ringer lactate from the lower hook.

Wait until the selected mode *– P.B., G.B.1 or G.B.2–* stops blinking.

Once the bottle is in place and the screen stops blinking, lift the bottle and the alarm should sound.
If so, you are “Ok to go”!

When the B.S.S. levels are low an alarm will beep. Don’t set up the device again! Just change the bag or bottle.